



i-LiNQ[®] Implant

i-LiNQ[®] Implant.



TWO Different Philosophies
ONE Single Implant.

i-LiNQ[®] Implant.

i-LiNQ[®] Implant is the biO₂logic consequence from the morphologic benefit of vascularized bone inside the outlines of the implant and the inductive effect of function based bone healing. The vascularized Havers'sian like bone morphology provides high oxygen supply and a fast structural adaptability on loading forces applied to bone under function.

Combining these two different philosophies in one single implant makes i-LiNQ[®] Implant safe, predictable and easy to use.

i-LiNQ[®] Implant.



1 Evaluation of transversal bone profile

For selecting the implant diameter please make sure that on both sides, vestibularity and orally, sufficient bone layer of at least 1 mm should remain.

© ImplantConcept GmbH

2 Minimally invasive access and pilot osteotomy

» 50 rpm without or » 600 rpm with irrigation

Pilot drill 2.0 mm

© ImplantConcept GmbH

3 Position-, depth- and axis-check

8 mm
6 mm
5 mm
4 mm

© ImplantConcept GmbH

4 Start „Low-Speed Drilling Protocol“

Check correct depth of osteotomy.

15 mm
14 mm
12 mm
11 mm
10 mm
9 mm
8 mm

© ImplantConcept GmbH

5 Drill to Implantat selection

Bone Quality			
Drill	D1 / D2	D 3	D 4
2.5	2.7	3.0	3.5
2.8	3.0	3.5	4.0
3.3	3.5	4.0	4.5
3.7	4.0	4.5	5.0
4.2	4.5	5.0	5.5
4.7	5.0	5.5	6.0

Implant Diameter

© ImplantConcept GmbH

6 Final drill diameter should be corresponding to bone quality

Re-check for correct depth of osteotomy.

© ImplantConcept GmbH

Clinical Protocol: i-LiNQ® Implant

Clinical Protocol: i-LiNQ® Implant

7 Bone chips collection

Bone chips, harvested by „Low-Speed-Drilling Protocol“: ready for augmentation.

© ImplantConcept GmbH

8 Implant insertion

≤ 30 U/min
≤ 50 Ncm

© ImplantConcept GmbH

9 Insertion tool removal

Healing chambers for Haversian like vascularized bone formation.

High primary stability by „Bionic Threads Design“.

© ImplantConcept GmbH

10 Crestal volume support

Place the bone chips into the circular gap between i-LiNQ® and osteotomy. Do not overextend!

© ImplantConcept GmbH

11 Wound closure

Atraumatic suture material is appropriate. We recommend ATRAMAT® PGC 25 in gauge 4-0, 5-0 und 6-0. Equipped with the outstanding Atraglide® needle, PGC 25 in size 13 and 16 mm is ideally suitable.

© ImplantConcept GmbH

12 i-LiNQ® – more options.

© ImplantConcept GmbH

i-LiNQ® Implant 2.7



2.7 mm

L

8
10
12
14

I-MF 2708
I-MF 2710
I-MF 2712
I-MF 2714

i-LiNQ® Implant 3.0



3.0 mm

L

8
10
12
14

I-MF 3008
I-MF 3010
I-MF 3012
I-MF 3014

i-LiNQ® Implant 3.5



3.5 mm

L

8
10
12
14

I-MF 3508
I-MF 3510
I-MF 3512
I-MF 3514

i-LiNQ® Implant 4.0



4.0 mm

L

8
10
12
14

I-MF 4008
I-MF 4010
I-MF 4012
I-MF 4014

i-LiNQ® Implant 4.5



4.5 mm

L

8
10
12
14

I-MF 4508
I-MF 4510
I-MF 4512
I-MF 4514

i-LiNQ® Implant 5.0



5.0 mm

L

8
10
12

I-MF 5008
I-MF 5010
I-MF 5012

i-LiNQ® Implant 5.5



5.5 mm

L

8
10
12

I-MF 5508
I-MF 5510
I-MF 5512

i-LiNQ® Implant 6.0




6.0 mm

L

8
10
12

I-MF 6008
I-MF 6010
I-MF 6012

i-LiNQ® Implant.

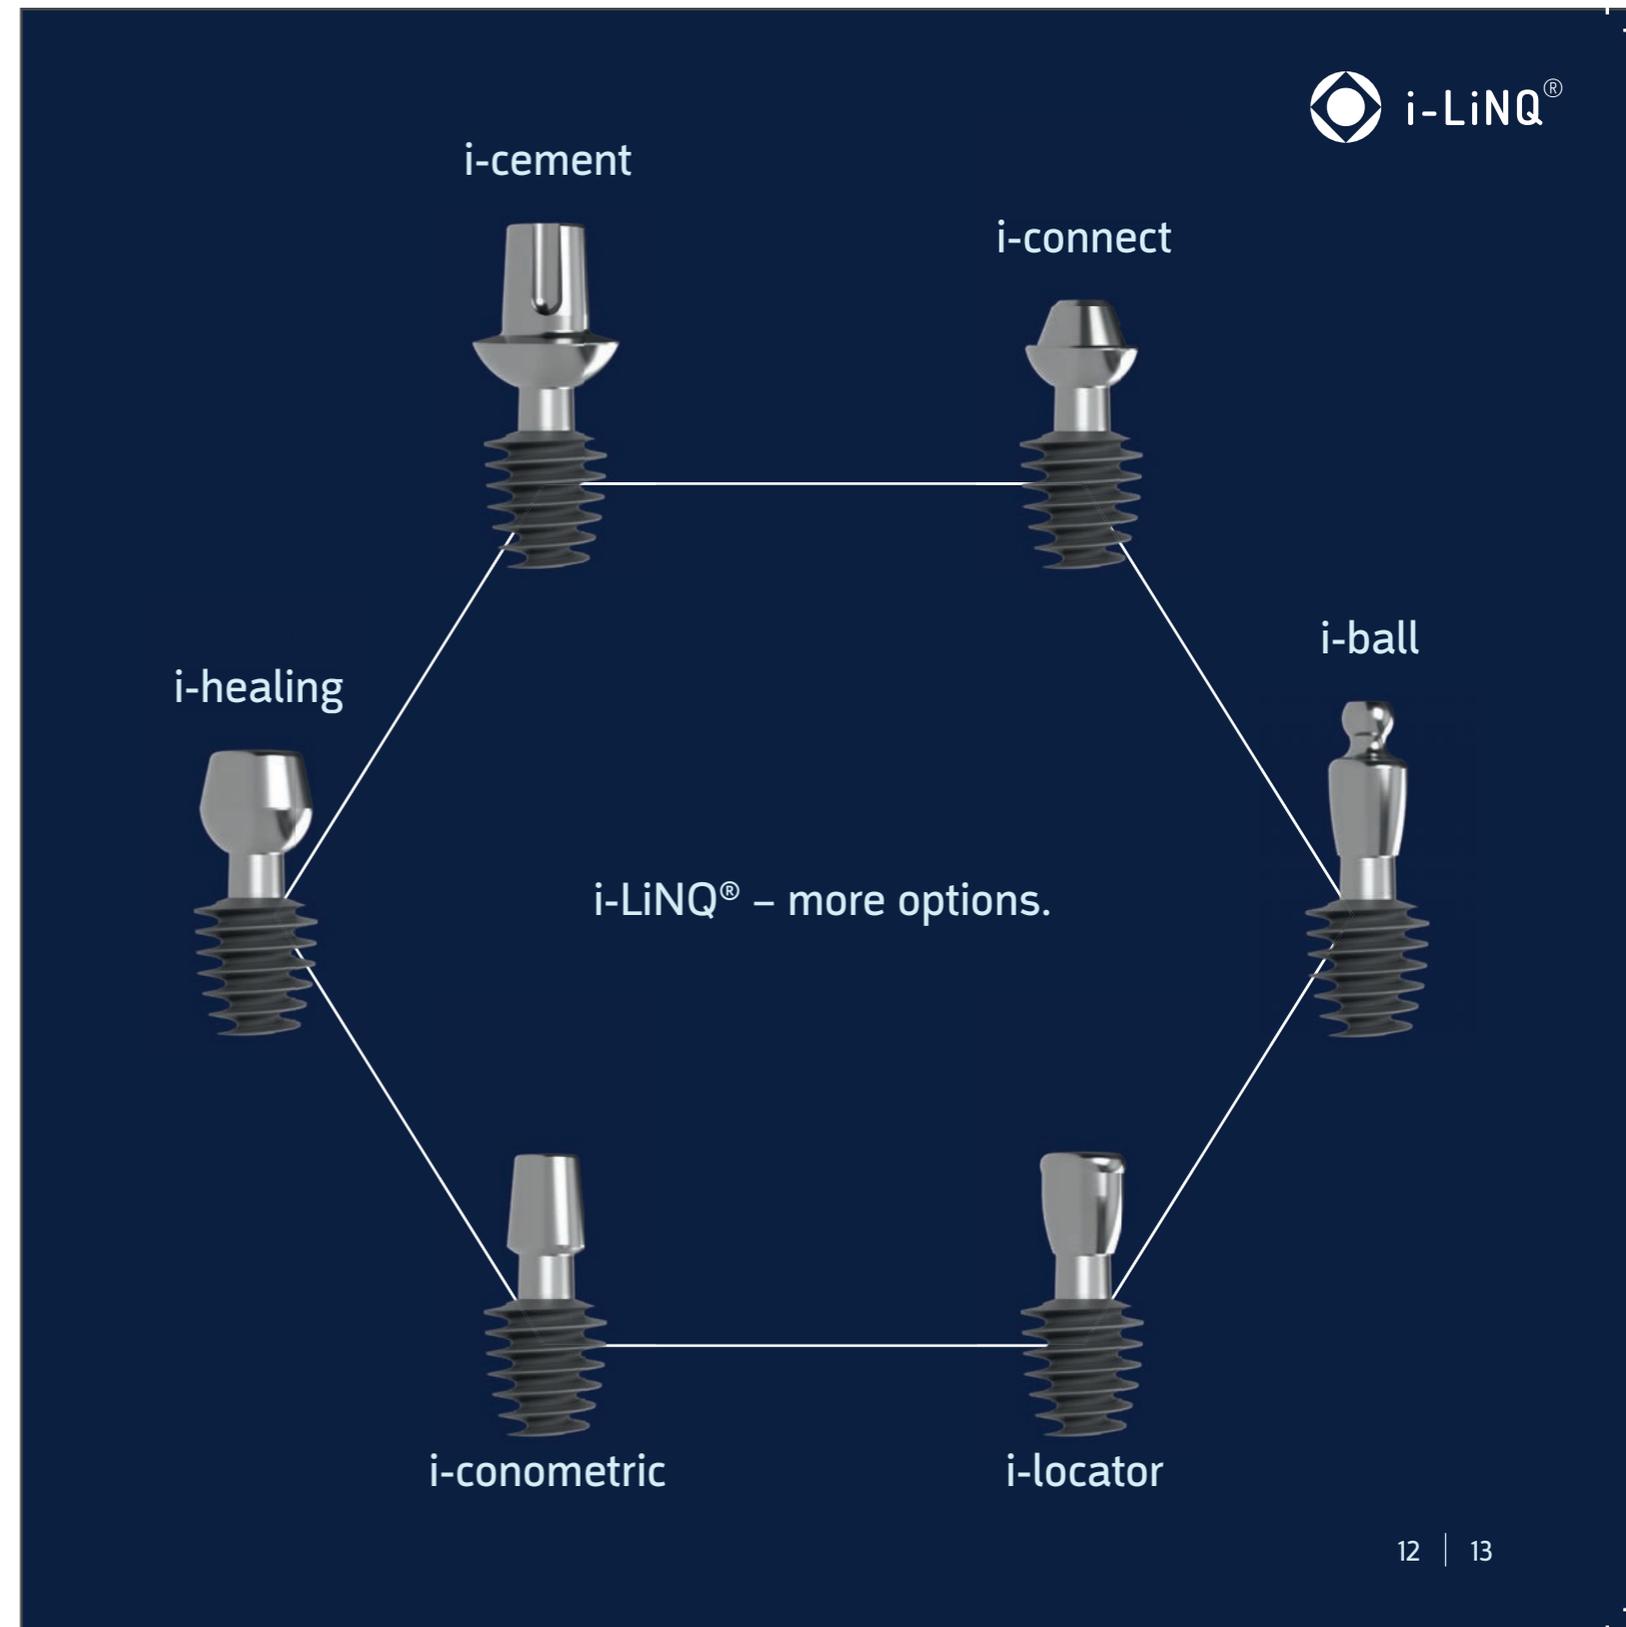



Editor: Novodent SA
legally represented by general manager Bernard Jahrmann
Avenue des Sciences 11, Y-Parc Technopole
CH-1400 Yverdon-les-Bains (Switzerland)
Phone: +41 24 524 28 28
email: info@isystemimplant.com
Registered with the commercial register of Vaud under
CHE-287.655.434

Text: Dr. Stefan König, M.Sc. M.Sc.
Design: Dr. Stefan König, M.Sc. M.Sc.
3-D-Rendering: Assoc. Prof. Nejat Nizam
Graphics: Dr. Stefan König, M.Sc. M.Sc.
Images: © Dr. Stefan König, M.Sc. M.Sc.

Published: 2021

Tous droits réservés.

La reproduction, également l'extrait et la reproduction de photos, n'est autorisée qu'avec l'autorisation écrite de ImplantConcept GmbH, Bochum/Allemagne.
Toutes les offres, commandes et livraisons sont soumises aux conditions générales de vente et de livraison, disponibles sur www.implant-concept.de.
Nous nous réservons le droit de modifier notre gamme de produits et leur design ainsi que de dévier des illustrations et données y figurant.

All rights reserved.

Reproduction, also by extract and reproducing photos, are only permitted by written authorisation of ImplantConcept GmbH, Bochum/Germany.
All offers, orders, and deliveries are subject to „General Sales and Delivery Terms“, available on www.implant-concept.de.
We reserve the right to modify our range of products and their design as well as to deviate from the illustrations and data shown.

© 2021 – ImplantConcept GmbH



NOVODENT

Avenue des Sciences 11 • Y-Parc Technopole
CH-1400 Yverdon-les Bains (Switzerland)
Phone: +41 24 524 28 28
ilinqimplant.com